

Peripheral catheter directed thrombolysis (CDT) with alteplase Clinical Guideline

Version No.: V1.1

Approval date: 20 March 2023



Government
of South Australia

SA Health

Contents

1.	Introduction	3
2.	Background	3
3.	Definitions	3
4.	Principles of the standards	3
5.	Safety, quality and risk management	4
6.	Pathway / Protocol	4
6.1	Contraindications/Precautions	5
6.2	Preparation	6
6.3	Procedure	6
6.4	Dosage	7
6.5	Observations	8
6.6	Adverse reactions	9
7.	Reference	9
8.	Document Ownership & History	10

Peripheral catheter directed thrombolysis (CDT) with alteplase Clinical Guideline

1. Introduction

Alteplase is a thrombolytic medication used for the dissolution of arterial or venous, thrombus or emboli. Peripheral catheter directed thrombolysis (CDT) is a procedure used to deliver the thrombolytic directly to the location of the thrombus/embolus.

2. Background

This guideline has been developed jointly by the Vascular Surgery Departments of SALHN and CALHN to assist in the safe administration and management of alteplase during peripheral catheter directed thrombolysis.

The use of alteplase for catheter directed thrombolysis is an 'off-label' indication. The following guideline has been developed based on primary literature, published guidelines, expert opinion and clinical experience.

3. Definitions

CDT: Catheter directed thrombolysis
 TIA: Transient ischaemic attack
 CPR: Cardiopulmonary resuscitation
 FBC: Full blood count
 EUC: Electrolytes, urea & creatinine
 LFT: Liver function test
 APTT: Activated partial thromboplastin time
 INR: International normalised ratio
 SBP: Systolic blood pressure
 PE: Pulmonary embolus
 SALHN: Southern Adelaide Local Health Network
 CALHN: Central Adelaide Local Health Network

4. Principles of the standards

The following National Safety and Quality Health Service Standards apply:

Standard 1- Governance for Safety and Quality in Health Care

Create integrated governance systems that maintain and improve the reliability and quality of patient care, as well as improve patient outcomes.

Standard 4- Medication Safety

Ensure competent clinicians safely prescribe, dispense and administer appropriate medicines to informed patients and carers.

5. Safety, quality and risk management

National Safety and Quality Health Service Standards

							
National Standard 1 Clinical Governance	National Standard 2 Partnering with Consumers	National Standard 3 Preventing & Controlling Healthcare-Associated Infection	National Standard 4 Medication Safety	National Standard 5 Comprehensive Care	National Standard 6 Communicating for Safety	National Standard 7 Blood Management	National Standard 8 Recognising & Responding to Acute Deterioration
☒	☐	☐	☒	☐	☐	☐	☐

6. Pathway / Protocol

Decision for CDT will be made by the treating consultant vascular surgeon.

Informed consent must be obtained (on a standard consent form) and a patient information leaflet should be provided: <http://www.anzsvs.org.au/patient-information/thrombolysis/>

GENERIC NAME: Alteplase

SYNONYMS: Recombinant tissue plasminogen activator, tPA

TRADE NAME: Actilyse®

PRESENTATION:

10mg vial of powder for dilution. Supplied with diluent vial of water for injection.
50mg not required for CDT.

CLINICAL USES:

Decision for CDT will be made by the treating consultant vascular surgeon.
Peripheral arterial thromboembolism
Deep vein thrombosis

ACTION:

Thrombolytic agent. Activates plasminogen by converting it to plasmin to initiate fibrinolysis.

6.1 Contraindications/Precautions

CONTRAINDICATIONS:

Absolute contraindications	Relative contraindications
• Hypersensitivity to alteplase, gentamicin or to the excipients • Active internal bleeding or disseminated intravascular coagulopathy • Significant bleeding disorder at present or within the past 6 months • Cerebrovascular event (including TIA), neurosurgery (intracranial or spinal) or intracranial trauma within the last 3 months • History of intracranial haemorrhage or subarachnoid haemorrhage • Intracranial neoplasm or other neoplasm with increased bleeding risk • Gastrointestinal bleeding within 10 days • Presence/development of compartment syndrome • Absolute contraindication to anticoagulation	• Severe uncontrolled hypertension (>160 systolic or >90 diastolic) • Arterial aneurysms, arterial/venous malformations (including cerebral) • Gastrointestinal bleeding >10 days and <3 months • Major surgery, trauma or CPR within 14 days (caution within 3 months) • Recent internal haemorrhage, puncture of non-compressible artery or organ biopsy • Recent eye surgery (<3 months) • Diabetic haemorrhagic retinopathy • Gastrointestinal diseases with potential sources of bleeding • Patients currently receiving oral anticoagulants eg warfarin, apixaban, rivaroxaban or dabigatran • Blood coagulation defects or thrombocytopenia (platelets <100x10⁹/L) • Severe hepatic insufficiency- decision made by treating consultant with consultation from liver specialist if required • Acute pancreatitis, pericarditis, bacterial endocarditis, sepsis or suspicion of septic emboli • Life expectancy < 1 year • Pregnancy or lactation

PRECAUTIONS:

- Access site complications are common during/after thrombolysis
 - Recommend care with arterial/venous access (ultrasound guidance recommended)
 - Manual compression of puncture site ≥30 minutes after cannula removal
 - Regular access site observations after compression
- Inability to tolerate prolonged arterial catheterisation eg unable to lie flat for a prolonged period of time (>12 hours) ie back pain, heart failure
- Severe renal impairment increases the risk of contrast induced acute kidney injury
 - Alteplase dose is unchanged in renal impairment³

6.2 Preparation

PREPARATION:

- Reconstitute 10mg vial with 10mL of the diluent provided. Add the diluent using the transfer cannula provided or a large bore needle (18 gauge). Swirl gently until completely dissolved. DO NOT SHAKE vigorously. Allow to stand for several minutes to dissipate large bubbles¹.
- The 10mg/10mL solution should be diluted in 500ml of 0.9% sodium chloride²
- Label bag as per labelling guidelines.

Resultant concentration 0.02mg/mL²

STABILITY:

Up to 24 hours at room temperature²

COMPATIBILITY:

0.9% Sodium chloride

Limited information. No other medication should be added to the prepared infusion solution¹.

BASELINE TESTS (prior to treatment):

Full blood count (FBC)

Coagulation studies (coags)

Group and save

Electrolytes, urea & creatinine (EUC), liver function tests (LFTs)

Observations- vascular, neurological, vital signs, temperature, pain score

6.3 Procedure

Preparation for CDT:

Prior to commencement of CDT

- 1) Ensure the shift coordinator of the receiving ward is aware of the planned CDT to arrange staffing allocation/requirements
- 2) IDC and 2 large bore IV lines to be placed

After CDT catheter placement in angiography suite

- 3) Catheter and sheath side arm to be labelled as per labelling guidelines in the angiography suite upon placement of lines
- 4) Vascular or interventional radiologist team performing procedure to prescribe alteplase infusion
- 5) Infusions to be connected in angiography recovery by the vascular surgeon, registrar or interventional radiologist and a senior nurse in concert with receiving ward nurse prior to transfer to the ward
- 6) Use only threaded lock cannula connections

Prior to transfer to receiving ward

- 7) Document medications to be withheld while patient receiving thrombolysis
- 8) Stress ulcer prophylaxis (eg pantoprazole 40mg daily, oral or IV) should be prescribed at initiation of thrombolysis and continued until discharge.

6.4 Dosage

CATHETER (intra-arterial or intra-venous)

Alteplase bolus:

5mg bolus, may repeat if required.

Maximum bolus of 20mg (ie 4x5mg bolus).

Alteplase infusion:

See 'Preparation' section on page 6 for preparation

Run at **25mL/hour** of diluted solution (=0.5mg/hour)

Rate may be increased to a maximum of 50ml/hr of diluted solution (=1mg/hr) at the discretion of the treating surgeon.

Note: Treatment for venous thromboembolism may require the higher dosing regimen at the discretion of the treating surgeon.

Maximum total dose: 50mg (including bolus doses)

SHEATH side arm

Heparin infusion, to prevent peri-catheter thrombus formation:

25,000units/50ml unfractionated heparin syringe (=500units/mL)

Run **heparin** at **1mL/hour** (=500units/hour)

'Piggy back' 500mL bag of 0.9% sodium chloride onto heparin syringe. (See instructions below)

Run saline at 10mL/hour

THIS IS A SUBTHERAPEUTIC INFUSION. APTT SHOULD NOT BE THERAPEUTIC.

Reduce rate if APTT>60 seconds (consult vascular registrar)


This heparin infusion must be prescribed on a variable dose infusion chart or fluid chart.

Do not use "heparin infusion chart for systemic anticoagulation".

Therapeutic anticoagulation is not recommended while using alteplase CDT for venous thromboembolism^{16,20,45,47}

Instructions for set up of heparin syringe with saline 'piggy back':

1. Attach heparin syringe and prime microbore line
2. Attach microbore line to interlink extension with non- return valve on the non- valve/clamp side
3. Prime interlink extension to y-site with heparin
4. Prime pump line with 0.9% sodium chloride
5. Attach pump line to interlink extension with non-return valve on the valve side
6. Finish priming extension with sodium chloride
7. Attach distal end of pump line to the sheath side arm
8. Commence heparin and sodium chloride infusions

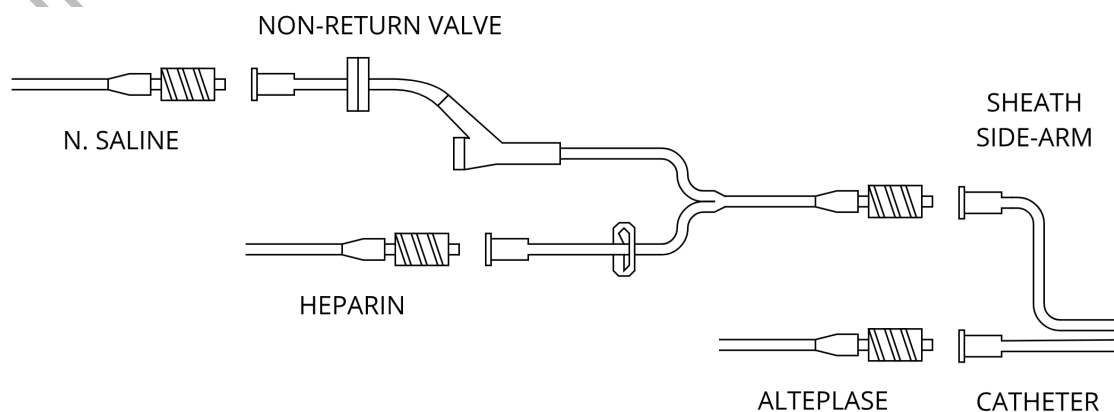

Note:

- Alteplase and heparin are incompatible via the same access device due to precipitation.
- Do not give oral anticoagulants (warfarin, apixaban, rivaroxaban or dabigatran) or low molecular weight heparin (enoxaparin or dalteparin) while running CDT due to the increased risk of haemorrhage.
- Do not give IM injections while undergoing CDT and for 24 hours after cessation.

6.5 Observations**Monitoring during CDT infusion:**

- 1) Nurse to patient ratio is 1:1 for the first 4 hours then reassess for potential 1:2 ratio for duration of infusion
- 2) Ensure baseline tests have been performed- see 'Preparation' section on page 6
- 3) Check patient identification, infusion program and lines on return to ward- 2 nurse check
- 4) Rate changes and reference ranges under direct supervision of the vascular registrar on call.
- 5) All rate and bag changes to be checked by 2 nursing staff
- 6) Blood pressure to be taken manually
- 7) Patient must rest in bed and lie flat while catheter/sheath are in place.
- 8) Strict 2-3 hourly pressure area care, keeping affected limb with catheter in situ as straight as possible. Consider a pressure reducing mattress
- 9) Mobility orders after removal of catheter as per vascular team
- 10) Fluid balance chart

Observation	Frequency
Neurovascular observations of affected limb Monitor catheter insertion site for bleeding/haematoma Check all line connections	Every 15 minutes for 2 hours then every 30 minutes for 4 hours then if stable hourly
Blood pressure (manual), pulse, temperature, respiratory rate, neurological observations, pain score, sedation score	Hourly for 4 hours then if stable 4 hourly
Blood tests: EUC, FBC, APTT*, INR and fibrinogen level**	4 hours after return to ward and then daily (or as ordered by MO)

*If APTT therapeutic (>60sec) decrease rate of heparin infusion

**If fibrinogen <1g/L consider FFP, reducing dose or stopping thrombolysis

Complication	Action
Major bleeding or haemodynamic or neurologic instability	STOP INFUSION and notify vascular registrar immediately
Haemorrhage/haematoma at access site	Apply local pressure (no sandbag) and notify medical officer and vascular registrar immediately
Deteriorating neurovascular observations or increased pain in either limb	Notify vascular registrar
Tachycardia (pulse>100), hypertension (SBP>160mmHg) or headache	Notify vascular registrar

FOLLOW UP ANGIOGRAPHY:

Patient will require follow up angiography within 24 hours of thrombolysis initiation

Repeat check angiography every 24 hours while CDT continues

Check with registrar or consultant for hydration protocol

Patient to be fasted from solids for 2 hours prior (can have clear fluids) or as advised

Routine post angiography observations

6.6 Adverse reactions

Very Common: Haemorrhage (puncture site and wound)

Common: Haemorrhage (including intracerebral, gastrointestinal), haematuria, fever, chills, nausea, vomiting

Uncommon: epistaxis, hypotension, urticaria, bronchospasm

Rare: hypersensitivity/anaphylaxis (refer to local Anaphylaxis management guideline for treatment)

Unknown incidence: cholesterol embolism, embolism formed through thrombus degradation (including PE)

7. Reference

1. Australian Injectable Drugs Handbook, 7th Ed. Society of Hospital Pharmacists of Australia; 2017
2. Semba CP et al. Alteplase: Stability and Bioactivity after Dilution in Normal Saline Solution. *J Vasc Interv Radiol* 2003; 14:99-102
3. Activase (alteplase) product information, San Francisco, United States, Genentech; January 2017
4. Actilyse (alteplase) product information, United Kingdom, Boehringer Ingelheim Limited; April 2017
5. Agle SC, McNally MM, Powell et.al. The association of periprocedural hypertension and adverse outcomes in patients undergoing catheter-directed thrombolysis. *Ann Vasc Surg* 2010; 24: 609-614
6. Alteplase (rt-PA) and heparin infusion for catheter directed thrombolysis. The Leeds Teaching Hospitals, United Kingdom; 2012
7. Antithrombotic therapy in peripheral artery disease. Antithrombotic therapy and prevention of thrombosis, 9th ed. American College of Chest Physicians Evidence Based Clinical Practice Guidelines. *CHEST* 2012; 141(2):e669S-690S
8. Australian Injectable Drugs Handbook, 7th Ed. Society of Hospital Pharmacists of Australia; 2017
9. Baekgaard N, Broholm R, Just S et. al. Long-term results using catheter-directed thrombolysis in 103 lower limbs with acute iliofemoral venous thrombosis. *Eur J Vasc Surg* 2010; 39: 112-117
10. Baldwin ZK, Comerota AJ, Schwartz LB et. al. Catheter-directed thrombolysis for deep vein thrombosis. *Vasc Endovasc Surg*. 2004; 38: 1-9
11. Braithwaite BD, Buckenham TM, Galland RB et. al. on behalf of the Thrombolysis Study Group. Prospective randomised trial of high-dose bolus versus low-dose tissue plasminogen activator infusion in the management of acute limb ischaemia. *Br J Surg* 1997; 84: 646-650
12. Catheter directed thrombolysis for treatment of deep vein thrombosis or acute occlusive peripheral arterial disease for the adult patient, Procedure manual, Princess Alexandra Hospital, Brisbane, Australia; 2015
13. Casanegra AI, McBane RD, Bjarnason H. Intervention radiology for venous thrombosis: early thrombus removal using invasive methods. *British Journal of Haematology* 2017
14. Cina CS, Goh RH, Chan J et. al. Intraarterial catheter-directed thrombolysis: urokinase versus tissue plasminogen activator. *Ann Vasc Surg* 1999; 13: 571-575
15. Enden T, Haig Y, Klow N et. al. Long-term outcome after additional catheter-directed thrombolysis versus standard treatment for acute iliofemoral deep vein thrombosis (the CaVenT study): a randomised controlled trial. *Lancet* 2012; 379: 31-38
16. Enden T, Sandvik L, Klow N et. al. Catheter-directed venous thrombolysis in acute iliofemoral vein thrombosis- the CaVenT study: rationale and design of a multicentre, randomised, controlled, clinical trial (NCT00251771). *Am Heart J* 2007; 154: 808-814
17. Forster A, Wells P. Tissue plasminogen activator for the treatment of deep venous thrombosis of the lower extremity. A systematic review. *CHEST* 2001; 119: 572-579
18. Frazin B. Maximal dilution of Activase *American Journal of Hospital Pharmacy* 1990; 47: 1015
19. Garcia MJ, Lookstein R, Malhotra R et. al. Endovascular management of deep vein thrombosis with rheolytic thrombectomy: final report of the prospective multicentre PEARL (peripheral use of AngioJet rheolytic thrombectomy with a variety of catheter lengths) registry. *J Vasc Interv Radiol* 2015; 26: 777-785
20. Grip O, Kuoppala M, Acosta S et. al. Outcome and complications after intra-arterial thrombolysis for lower limb ischaemia with or without continuous heparin infusion. *BJS* 2014; 101: 1105-1112
21. Grunwald MR, Hormann LV. Comparison of urokinase, alteplase and reteplase for catheter-directed thrombolysis of deep venous thrombosis. *J Vasc Interv Radiol* 2004; 15: 347-352
22. Haig Y, Enden T, Grotta O et. al. Post thrombotic syndrome after catheter-directed thrombolysis for deep vein thrombosis (CaVenT): 5 year follow-up results of an open-label, randomised controlled trial. *Lancet Haematol* 2016; 3: e64-71
23. Hynes BG, Margry RJ, Ruggiero N et. al. Endovascular management of acute limb ischaemia. *Ann Vasc Surg* 2012; 26: 110-124
24. Intra-arterial and intra-venous thrombolysis guideline, Vascular surgery/vascular radiology. University Hospital of South Manchester, United Kingdom; 2017
25. Kessel DO, Berridge DC, Robertson I. Infusion techniques for peripheral arterial thrombolysis. *Cochrane Database of Systematic Reviews* 2004, Issue 1
26. Leung DA, Blitz LR, Nelson T et.al. Rheolytic pharmacomechanical thrombectomy for the management of acute limb ischaemia: Results from the PEARL registry. *J Endovasc Ther* 2015
27. Liew A, Douketis J. Catheter- directed thrombolysis for extensive iliofemoral deep vein thrombosis: review of literature and ongoing trials. *Expert Review of Cardiovascular Therapy* 2016; 14:2: 189-200
28. Lonsdale RJ, Berridge DC, Earnshaw JJ et. al. Recombinant tissue-type plasminogen activator is superior to streptokinase for local intra-arterial thrombolysis. *Br J Surg* 1992; 79: 272-275

29. Ouriel K, Gray B, Clair DG, Olin J. Complications associated with the use of urokinase and recombinant tissue plasminogen activator for catheter-directed peripheral arterial and venous thrombolysis. *JVIR* 2000; 11: 295-298
30. Ouriel K, Kandarpa K. Safety of thrombolytic therapy with urokinase or recombinant tissue plasminogen activator for peripheral arterial occlusion: A comprehensive compilation of published work. *J Endovasc Ther* 2004; 11: 436-466
31. Palfreyman SJ, Booth A, Michaels JA. A systematic review of intra-arterial thrombolytic therapy for lower limb ischaemia. *Eur J Vasc Endovasc Surg* 2000; 19: 143-157
32. Patel NH, Krishnamurthy VN, Kim S, et. al. Quality improvement guidelines for percutaneous management of acute lower-extremity ischaemia. Society of Interventional Radiology Standards of Practice Committee. *J Vasc Interv Radiol* 2013; 24: 3-15
33. Peden E, Zhou W, Bush R et. al. The case for thrombolysis for iliofemoral venous thrombosis. *Semin Vasc Surg* 2005; 18: 139-147
34. Plate G, Jansson I, Forsell C et.al. Thrombolysis for acute lower limb ischaemia- A prospective, randomised, multicentre study comparing two strategies. *Eur J Vasc Endovasc Surg* 2006; 31: 651-660
35. Robertson I, Kessel DO, Berridge DC. Fibrinolytic agents for peripheral arterial occlusion. *Cochrane Database of Systematic Reviews* 2013, Issue 12
36. Sander S, White CM, Coleman CI. Comparative safety and efficacy of urokinase and recombinant tissue plasminogen activator for peripheral arterial occlusion: A meta-analysis. *Pharmacotherapy* 2006; 26(1): 51-60
37. Sebastian AJ, Robinson GJ, Dyet JF, Ettles DF. Long-term outcomes of low-dose catheter-directed thrombolytic therapy: A 5 year single-centre experience. *J Vasc Interv Radiol* 2010; 21: 1004-1010
38. Semba CP, Murphy TP, Bakal CW, et. al. Thrombolytic therapy with use of alteplase (rt-PA) in peripheral arterial occlusive disease: review of the clinical literature. *JVIR* 2000; 11: 149-161
39. Semba CP, Bakal CW, Calis KA, et. al. Alteplase as an alternative to urokinase. *JVIR* 2000; 11: 279-287
40. Sharifi M, Mehdipour, Bay C et. al. Endovenous therapy for deep vein thrombosis: the TORPEDO trial. *Catheterisation and Cardiovascular Interventions* 2010; 76: 316-325
41. Shortell CK, Queiroz R, Jahansson M et.al. Safety and efficacy of limited dose tissue plasminogen activator in acute vascular occlusion. *J Vasc Surg* 2001; 34: 854-859
42. Sillesen H, Just S, Jorgensen M, Baekgaard N. Catheter-directed thrombolysis for treatment of iliofemoral deep venous thrombosis is durable, preserves venous valve function and may prevent chronic venous insufficiency. *Eur J Vasc Surg* 2005; 30: 556-562
43. Sugimoto K, Hofmann LV, Razavi MK et. al. The safety, efficacy and pharmacoeconomics of low-dose alteplase compared with urokinase for catheter-directed thrombolysis of arterial and venous occlusions. *J Vasc Surg* 2003; 37: 512-517
44. The STILE investigators. Results of a prospective randomised trial evaluating surgery versus thrombolysis for ischaemia of the lower extremity. *Ann Surg* 1994; 3: 251-268
45. Vedantham S, Sista AK, Klein SJ et. al. for the Society of Interventional Radiology and Cardiovascular & Interventional Radiological Society of Europe Standards of Practice Committees. Quality improvement guidelines for the treatment of lower-extremity deep vein thrombosis with use of endovascular thrombus removal. *J Vasc Interv Radiol* 2014; 25: 1317-1325
46. Vedantham S, Goldhaber SZ, Kahn SR et. al. Rationale and design of the ATTRACT study- A multicentre randomised trial to evaluate pharmacomechanical catheter-directed thrombolysis for the prevention of post-thrombotic syndrome in patients with proximal deep vein thrombosis. *Am Heart J* 2013; 165(4): 523-530
47. Vedantham S, Thorpe PE, Cardella JF, et. al. for the Society of Interventional Radiology and Cardiovascular & Interventional Radiological Society of Europe Standards of Practice Committees. Quality improvement guidelines for the treatment of lower-extremity deep vein thrombosis with use of endovascular thrombus removal *J Vasc Interv Radiol* 2006; 17: 435-448
48. Vedantham S, Millward SF, Cardella JF, et. al. Society of Interventional Radiology Position Statement: treatment of acute iliofemoral deep vein thrombosis with use of adjunctive catheter-directed intrathrombus thrombolysis *J Vasc Interv Radiol* 2006; 17: 613-616
49. Ward AS, Andaz SK, Bygrace S. Peripheral thrombolysis with tissue plasminogen activator. Results of two treatment regimens. *Arch Surg* 1994; 139: 861-865
50. Watson L, Broderick C, Armon MP. Thrombolysis for acute deep vein thrombosis. *Cochrane Database of Systematic Reviews* 2014; Issue 1
51. Working Party on Thrombolysis in the Management of Limb Ischaemia. Thrombolysis in the management of lower limb peripheral arterial occlusion- A consensus document. *J Vasc Interv Radiol*. 2003; 7: S337-349

8. Document Ownership & History

Developed by:	Department of Vascular and Endovascular Surgery, Flinders Medical Centre, SALHN. Department of Pharmacy, SALHN. Department of Vascular Surgery, Royal Adelaide Hospital, CALHN
Contact:	Laura Brook
Endorsed by:	Domain Custodians, Clinical Governance, Safety and Quality
Next review due:	01/04/2024
ISBN number:	978-1-76083-267-4
CGSQ reference:	CG335
CG history:	Is this a new clinical guideline (V1)? N Does this clinical guideline amend or update an existing clinical guideline? Y If so, which version? Version 1 Does this clinical guideline replace another clinical guideline with a different title? N

Approval Date	Version	Who approved New/Revised Version	Reason for Change
20/03/2023	V1.1	Domain Custodians, Clinical Governance, Safety and Quality	Desktop review undertaken with no amendments
13/4/2020	V1	Deputy Chief Executive, Commissioning and Performance	Original approved version